



CERTIFICATE OF ACCREDITATION

The ANSI National Accreditation Board

Hereby attests that

Eurofins Infinity Laboratory Group Inc.

2250 Welsch Industrial Ct.

St. Louis, MO 63146

Fulfills the requirements of

ISO/IEC 17025:2017

In the field of

TESTING AND CALIBRATION

This certificate is valid only when accompanied by a current scope of accreditation document.
The current scope of accreditation can be verified at www.anab.org.

Jason Stine, Vice President

Expiry Date: 28 November 2027

Certificate Number: ACT-3262



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory
quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017

Eurofins Infinity Laboratory Group Inc.

2250 Welsch Industrial Ct.
St. Louis, MO 63146

Jennifer Eagan 557-219-1650
jennifer.eagan@bpt.eurofinsus.com

TESTING AND CALIBRATION

ISO/IEC 17025 Accreditation Granted: **24 November 2025**

Certificate Number: **ACT-3262**

Certificate Expiry Date: **28 November 2027**

TESTING

Chemical

Specific Tests and/or Properties Measured	Specification, Standard, Method, or Test Technique	Items, Materials, or Product Tested	Key Equipment or Technology
Extractables Testing	M230003 ISO 10993-18 & 11979-5 Chemical Characterization: ICP-MS Elemental Extractables	Various Medical Device Extractable Solutions	ICP-MS
Extractables Testing	M230005 ISO 10993-18 & 11979-5 Characterization: LC/UV/MS Extractables	Various Medical Device Extractable Solutions	LC-MS
Extractables Testing	M230006 ISO 10993-18 & 11979-5 Chemical Characterization: GC-MS Headspace Extractables	Various Medical Device Extractable Solutions	Headspace GC-FID

CALIBRATION


Mass and Mass Related

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Pipettes	Up to 1 µl (> 1 to 2) µl (> 2 to 10) µl (> 10 to 20) µl (> 20 to 100) µl (> 100 to 200) µl (> 200 to 1 000) µL	0.27 µL 0.27 µL 0.29 µL 0.32 µL 0.58 µL 1.7 µL 1.5 µL	Gravimetric Method using Electronic Balance; Based on ISO 8655-6: 2022 M25001-SL

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ($k=2$), corresponding to a confidence level of approximately 95%.

Notes:

- 1) The Scope Uncertainty presented here is the best measurement capability that the laboratory can achieve. The actual measurement uncertainty (MU) reported on a calibration certificate by the laboratory will be greater than or equal to the scope uncertainty presented here due to the behavior of the unit under calibration and influences of specific circumstances of the calibration.
- 2) The type of measurement or material being calibrated is defined by the parameter. This indicates the laboratory is capable of calibrating instruments that measure or generate the values in the ranges indicated for the parameter.

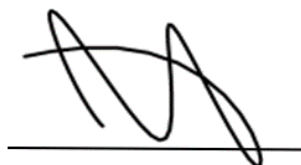

Jason Stine, Vice President